Blood glucose meter with Bluetooth transmission
G-427B

6.8
mmol/L
11-16
2:08PM

Fast **Exact** **Stable**

Less blood sample，fast and stable testing

0.1ul blood sample.
only need 5 second from testing to evaluation.

5.8
mmol/L
2:08PM
11-16

Four electrode technique, Anti-interference , More Accurate

Better interference resistance of RBC accretion avoid the influence for testing result, make the measurement result more accurate.

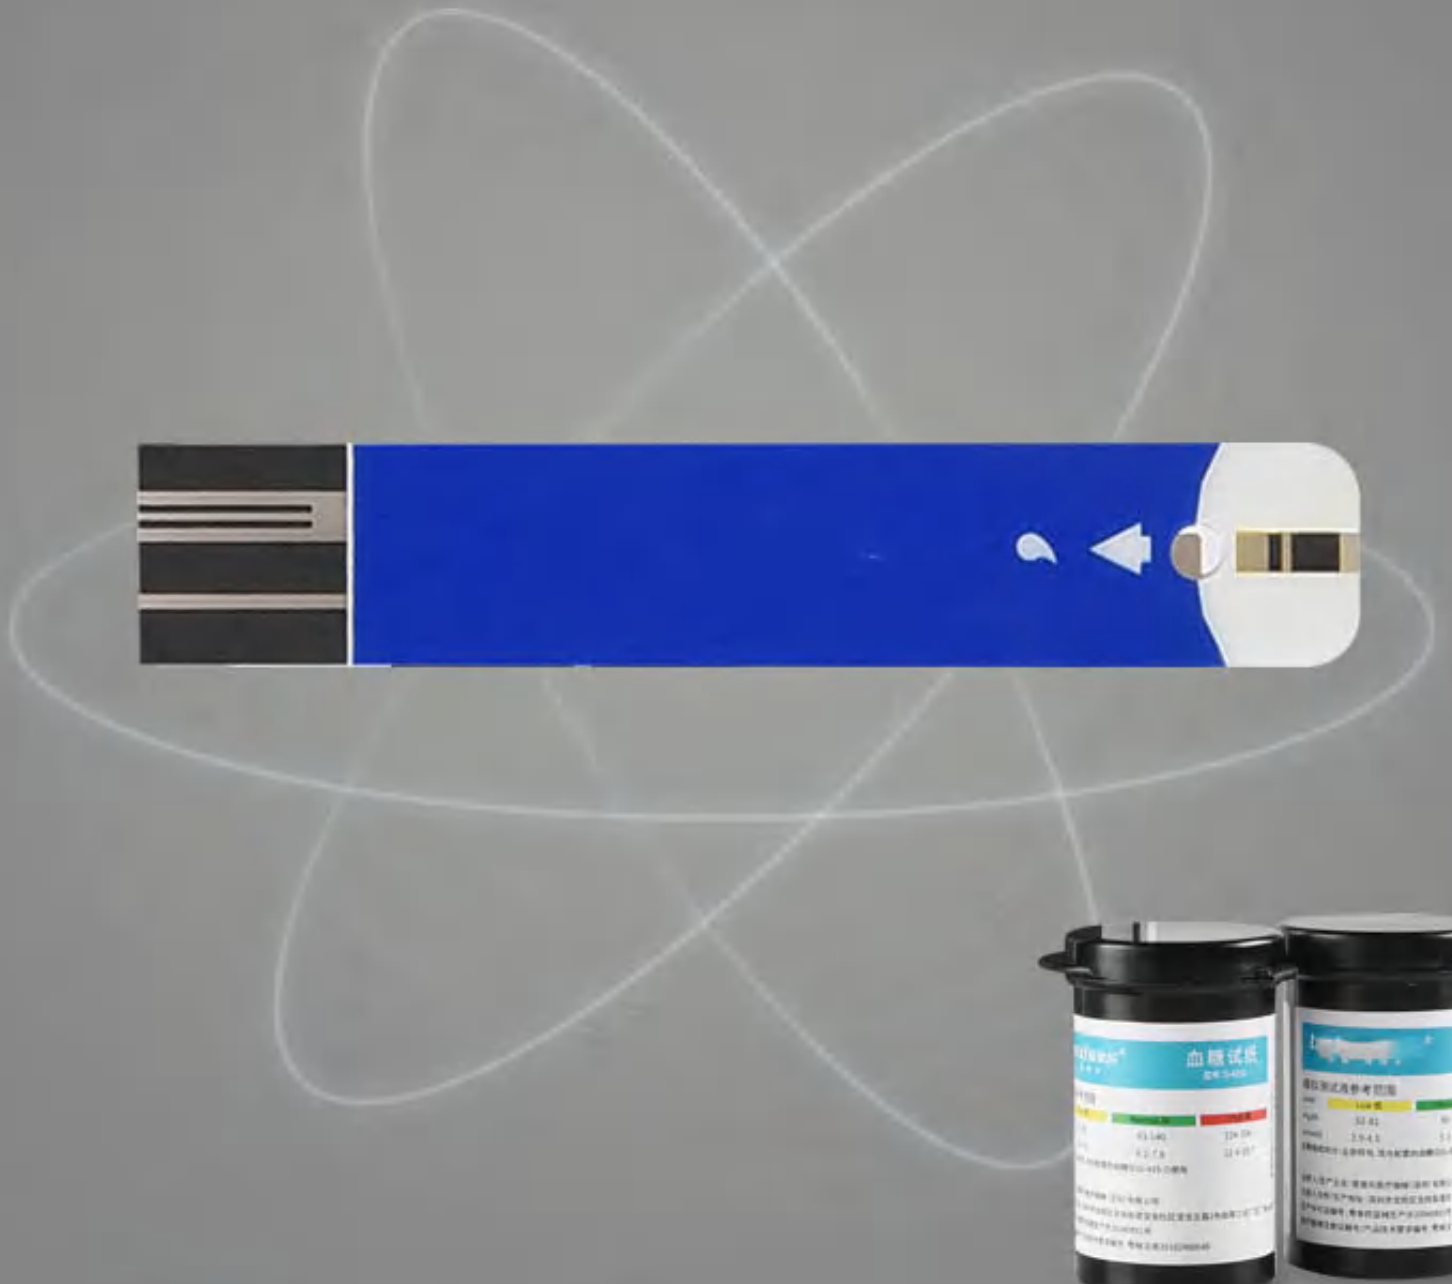

Large size LCD screen with back light for easy reading at night.

6.8
mmol/L
11-16 2:08 PM

Bluetooth 4.0 transmission ,

Intelligent Analysis to monitoring and controlling blood glucose

Overview of
blood pressure

Trend analysis

Blood
pressure record

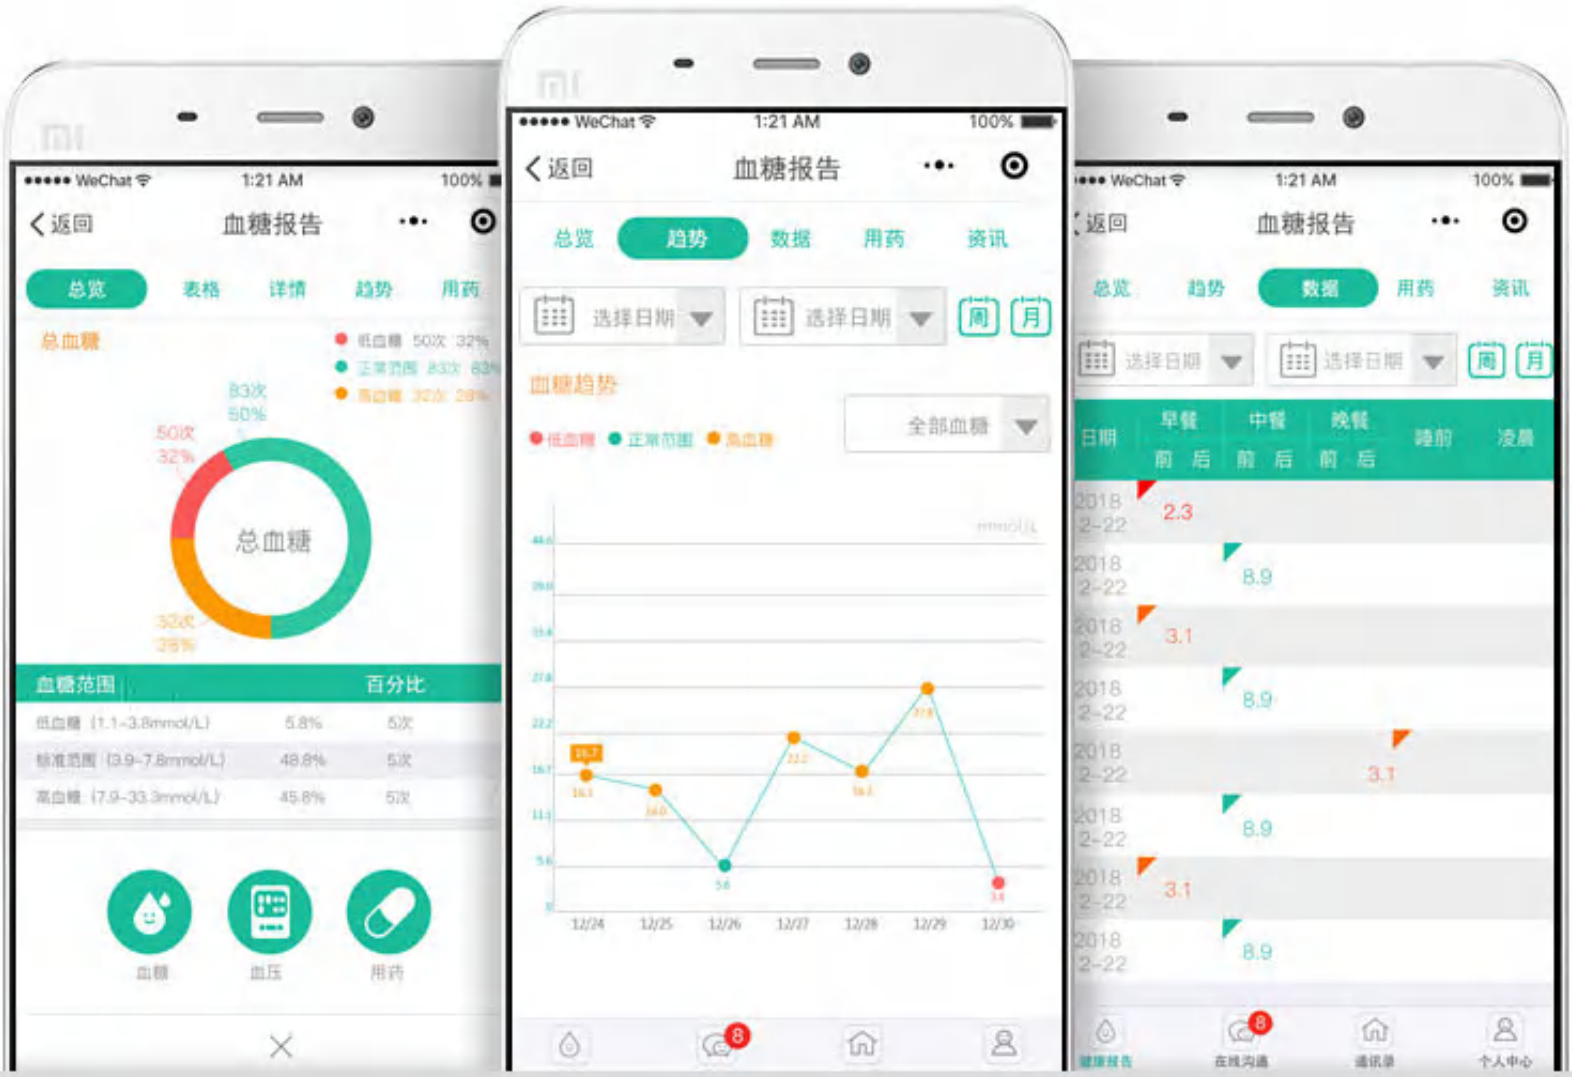
WeChat
1:21 AM
100%
返回
血糖报告
总览
表格
详情
趋势
用药
总血糖
低血糖 50次 32%
正常范围 83次 83%
高血糖 32次 28%
83次
50%
50次
32%
总血糖
32次
28%
血糖
血压
用药
返回
血糖报告
总览
趋势
数据
用药
资讯
选择日期
选择日期
周
月
血糖趋势
低血糖
正常范围
高血糖
全部血糖
mmol/L
27.8
22.2
16.7
11.1
5.6
0
16.7
5.6
22.2
27.8
12/24
12/25
12/26
12/27
12/28
12/29
12/30
8
返回
血糖报告
总览
趋势
数据
用药
资讯
选择日期
选择日期
周
月
8
健康报告
在线沟通
通讯录
个人中心

血糖范围	百分比	
低血糖（1.1~3.8mmol/L）	5.8%	5次
标准范围（3.9~7.8mmol/L）	48.8%	5次
高血糖（7.9~33.3mmol/L）	45.8%	5次

日期	早餐		中餐		晚餐		睡前	凌晨
	前	后	前	后	前	后		
2018 2-22	2.3							
2018 2-22			8.9					
2018 2-22	3.1							
2018 2-22			8.9					
2018 2-22							3.1	
2018 2-22			8.9					
2018 2-22	3.1							
2018 2-22			8.9					

The testing result can be shared with familes, friends and doctor, which will letting them better know the situation of blood glucose .

6.8
mmol/L
11-16 2:08PM

Bluetooth 4.0

Fasting blood-glucose 5.0mmol/L, let me share with others.

The blood-glucose result of Dad is good

Daughter

After made adjustment, the result is good . keep on to maintain this result.

Doctor

Will learn from him about how to control the blood-glucose so good.

Other patient

Considerate design for better using

448 Set memory

No Coding

Auto strip Ejection

Small size , easy to carry

BLOOD GLUCOSE METE

记忆
6-21 8:08
5.8
mmol/L

448sets Memory for easily observing Blood glucose trending

No Coding

Insert the strip, meter will recognize the strip automatically to avoid misdetecting caused by coding.

5.8
mmol/L
11-16 2:08PM

Auto strip Ejection

Press one button to eject strip automatically , no need to collect used strip. Convenient and sanitary

Small and portable, easy to carry and make test anytime and anywhere.

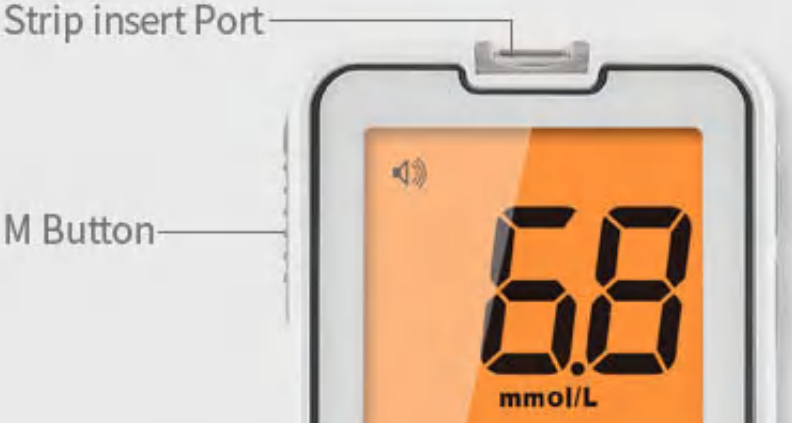
Strip insert Port
M Button
6.8
mmol/L

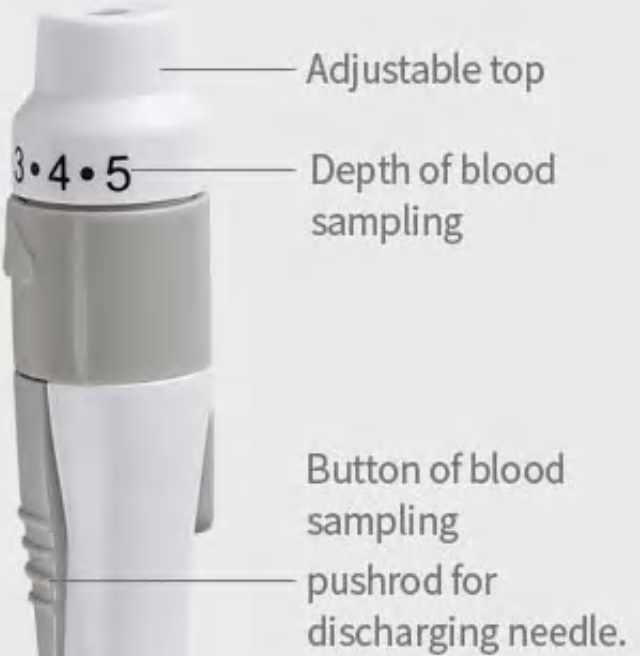
Adjustable top
3•4•5
Depth of blood sampling
Button of blood sampling
pushrod for discharging needle.

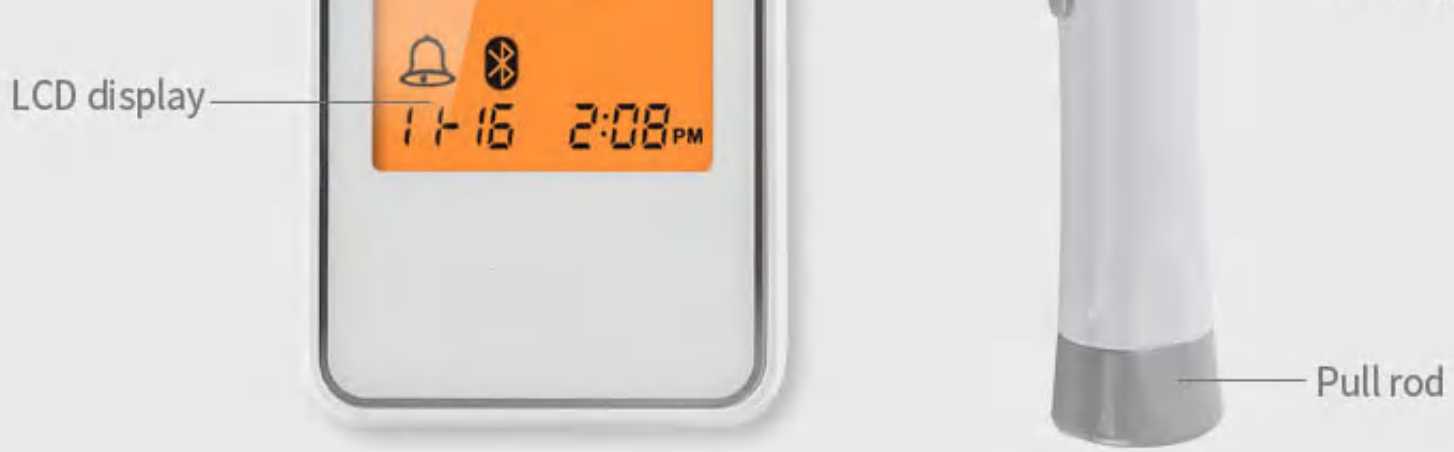
LCD display
11-16 2:08PM
Pull rod

Basic Parameter

Storage Environment	-20°C ~55°C, RH≦93%
Memory	448sets
Testing unit	mmol/L or mg/dL
Data Reading	LCD screen
Testing time	5S
Product size	90 x 54 x 13cm
Weight	73g (including battery)
Testing range	1.1 ~33.3mmol/L
Targe blood	Microvascular blood
Battery	2 x AAA Battery, DC3V

How to Use



01

Insert Test Strip



02

Blood sampling with lancet device



03

Use strip to contact the blood sample



04

Wait for 5S to see the testing result.

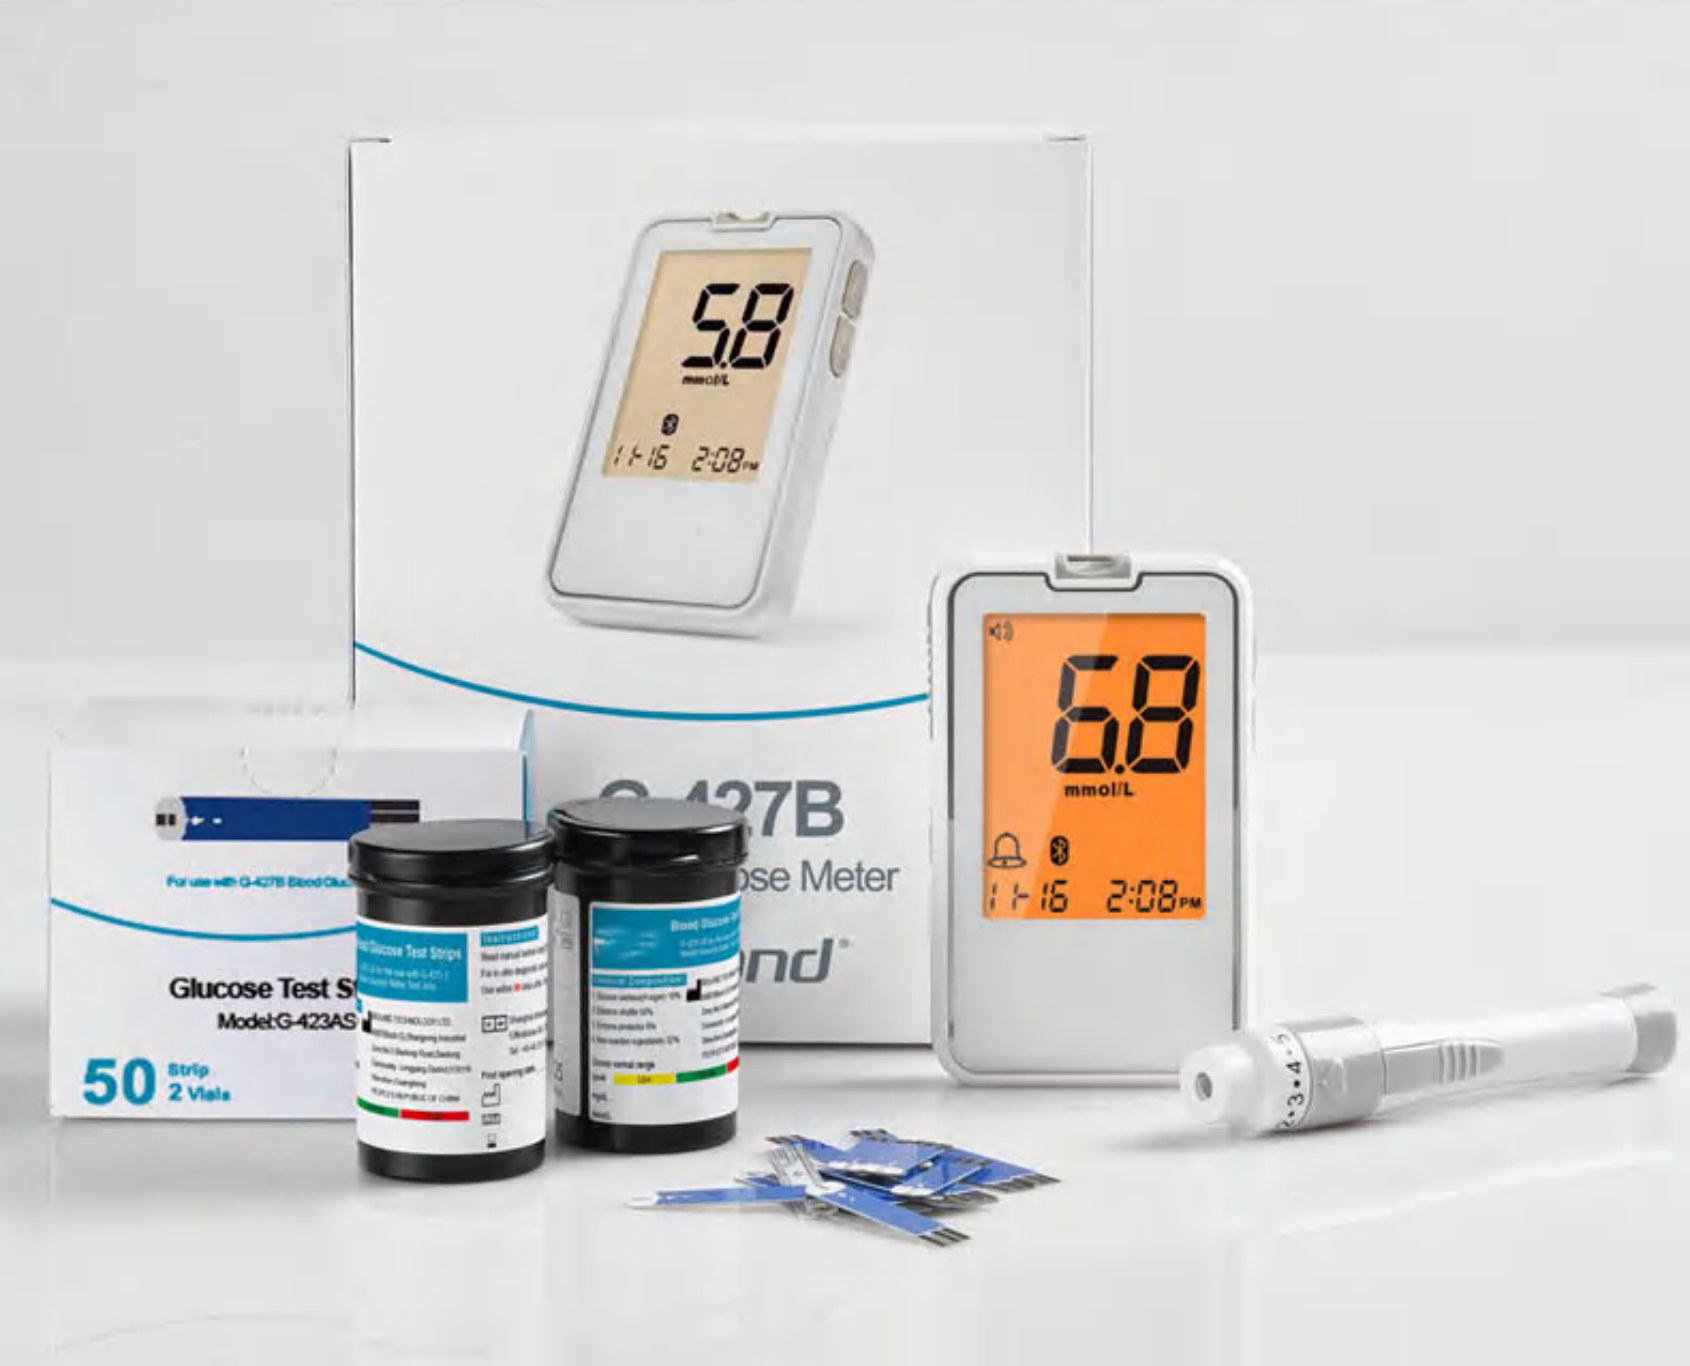
5.8
mmol/L
11-16 2:08PM
G-427B
Glucose Meter
6.8
mmol/L
11-16 2:08PM
For use with G-427B Blood Glucose
Glucose Test S
Model:G-423AS
50 Strip 2 Vials
Blood Glucose Test Strips